


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2130, Rack A, Plate 1, Well H03, 502912  
[CD37197F91B4AC40] Apr 24, 2026 14:09:07 Pressure = 61 bar (61 to 63)

FA

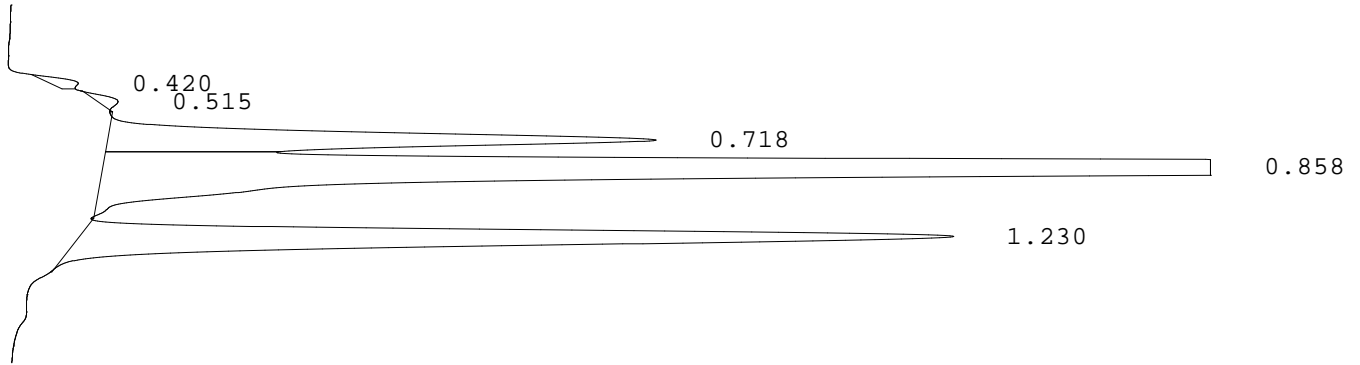

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.420	F 0.49	0.4%	8315	
2	0.515	F 0.60	0.4%	7857	
3	0.718	F 0.83	12.3%	244103	Acetylated F peak
4	0.858	F 1.00	66.0%	1304583	Consistent with F
5	1.230	A 1.00	20.9%	412946	A peak - REVIEW
Total Area: 1977804					

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range