


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2049, Rack A, Plate 1, Well D10, 490377
[C867D85F94EA0C40] Jan 20, 2026 12:32:03 Pressure = 80 bar (80 to 81)

FA

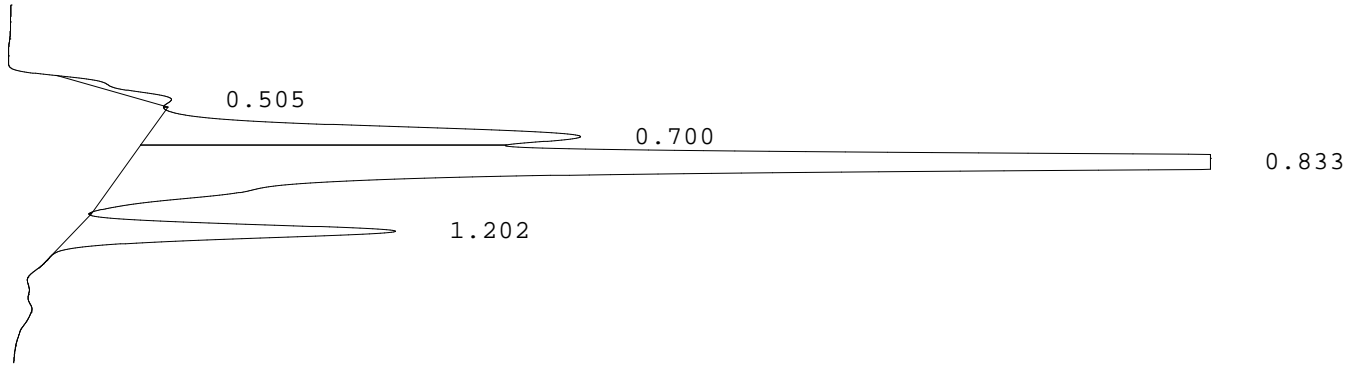

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.505	F 0.60	1.3%	20011	
2	0.700	F 0.83	15.5%	238504	Acetylated F peak
3	0.833	F 0.99	73.8%	1132836	Consistent with F
4	1.202	A 1.01	9.3%	143104	A peak
Total Area:				1534455	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range