


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2166, Rack A, Plate 1, Well B01, 501581  
[CD79B758B42719BF] Jun 02, 2026 10:26:20 Pressure = 64 bar (63 to 66)

FA

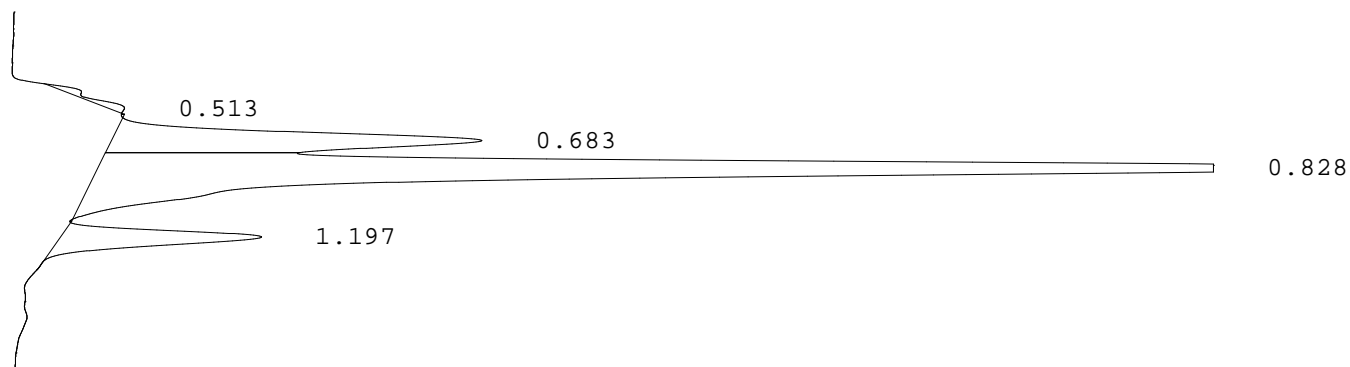

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.513	F 0.61	1.2%	11937	
2	0.683	F 0.82	18.9%	193598	Acetylated F peak
3	0.828	F 0.99	71.0%	725942	Consistent with F
4	1.197	A 1.01	8.9%	90807	A peak
Total Area:				1022284	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range