


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2054, Rack A, Plate 1, Well F10, 489175
[9D669A8AC2BF7395] Jan 26, 2026 13:03:23 Pressure = 86 bar (86 to 89)

FA

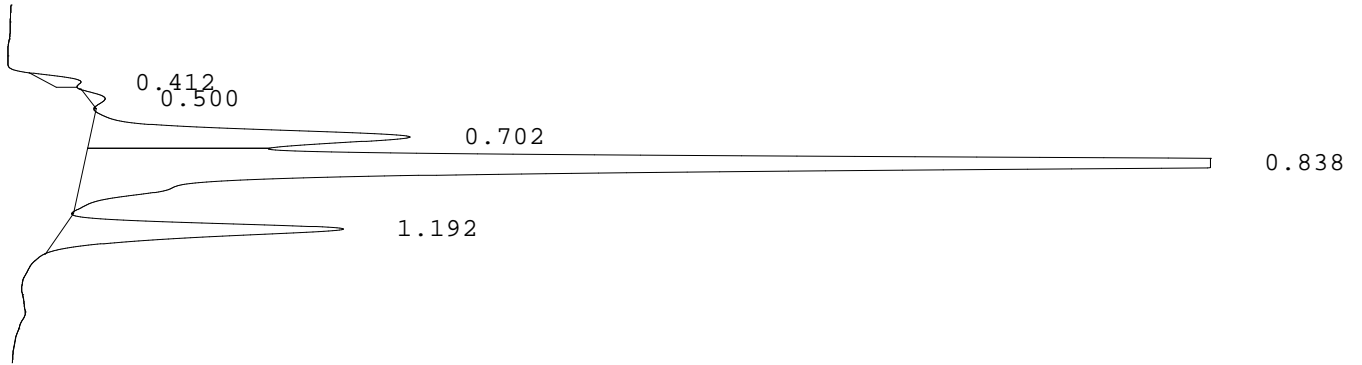

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.412	F 0.48	1.0%	10457	
2	0.500	F 0.58	0.6%	5837	
3	0.702	F 0.82	15.3%	158915	Acetylated F peak
4	0.838	F 0.98	71.5%	744751	Consistent with F
5	1.192	A 1.01	11.7%	121468	A peak
Total Area:				1041428	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range