


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1930, Rack A, Plate 1, Well F04, 478876
 [CD704DF40F36D19D] Oct 03, 2025 12:24:09 Pressure = 62 bar (62 to 63)

FA

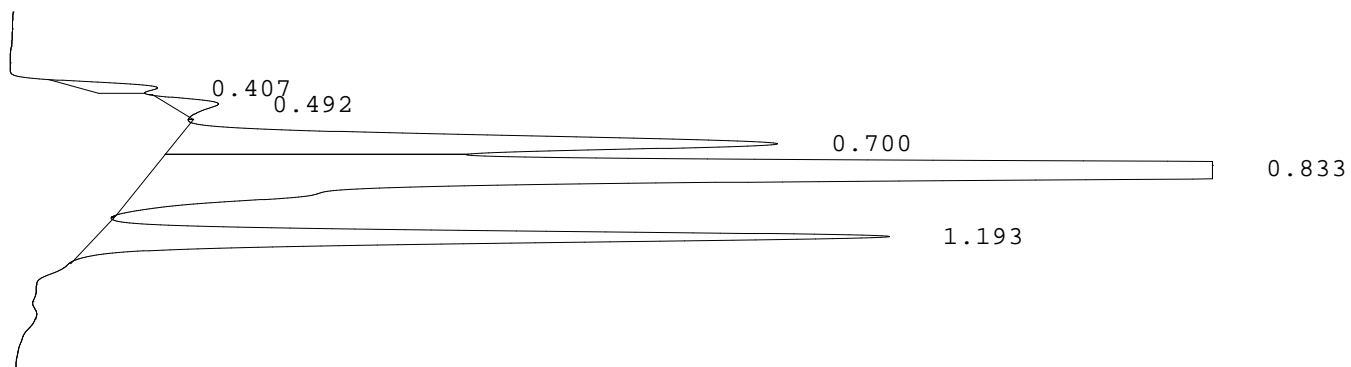

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	1.1%	22031	
2	0.492	F 0.58	1.0%	19608	
3	0.700	F 0.83	14.6%	294388	Acetylated F peak
4	0.833	F 0.99	68.1%	1370797	Consistent with F
5	1.193	A 1.00	15.2%	305961	A peak
Total Area:				2012785	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range