


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2098, Rack A, Plate 1, Well E02, 172655-p
[DC266F5401CE2448] Mar 19, 2026 12:54:57 Pressure = 60 bar (59 to 61)

FA

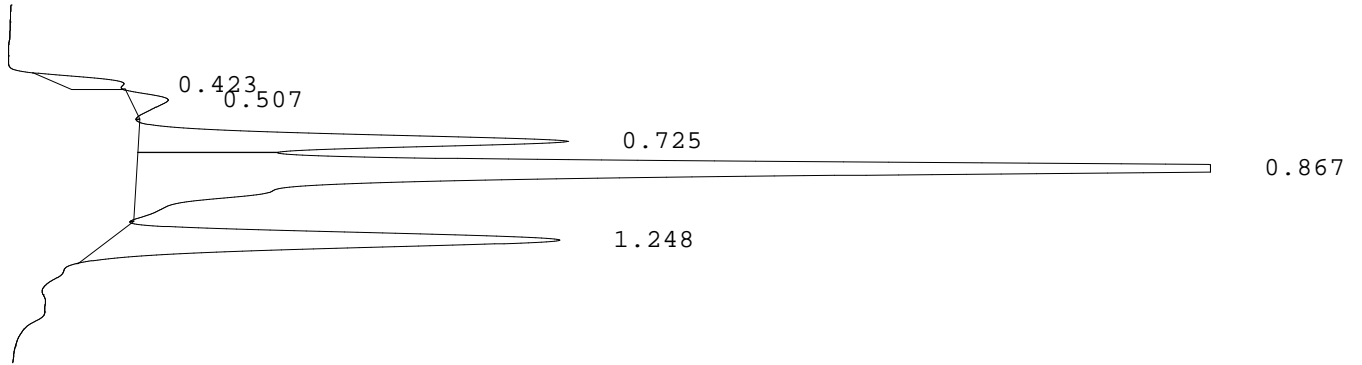

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.423	F 0.48	2.1%	22922	
2	0.507	F 0.57	1.6%	17562	
3	0.725	F 0.82	16.4%	180577	Acetylated F peak
4	0.867	F 0.98	59.9%	659452	Consistent with F
5	1.248	A 1.01	20.0%	220311	A peak
Total Area:				1100824	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range