


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 1967, Rack A, Plate 1, Well A03, 170875
[CD76A02ACE72ACE2] Nov 05, 2025 12:18:22 Pressure = 66 bar (66 to 68)

FA

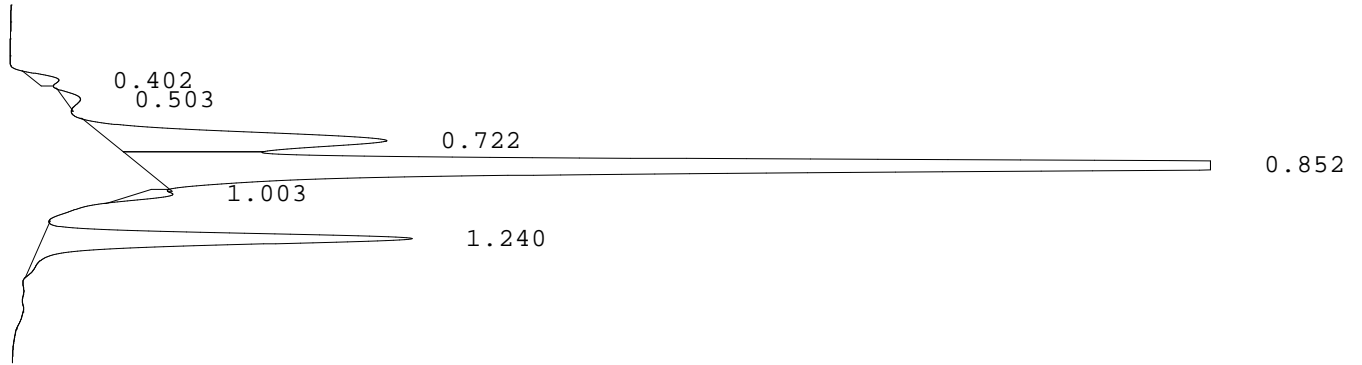

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.402	F 0.47	0.8%	7424	
2	0.503	F 0.58	0.7%	6361	
3	0.722	F 0.84	15.5%	141825	Acetylated F peak
4	0.852	F 0.99	66.9%	613261	Consistent with F
5	1.003	F 1.16	1.2%	11135	
6	1.240	A 1.00	15.0%	137139	A peak
Total Area:				917145	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range