


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2049, Rack A, Plate 1, Well A11, 498911  
[DC22C80AC3955B3D] Jan 20, 2026 11:19:17 Pressure = 81 bar (81 to 83)

FA

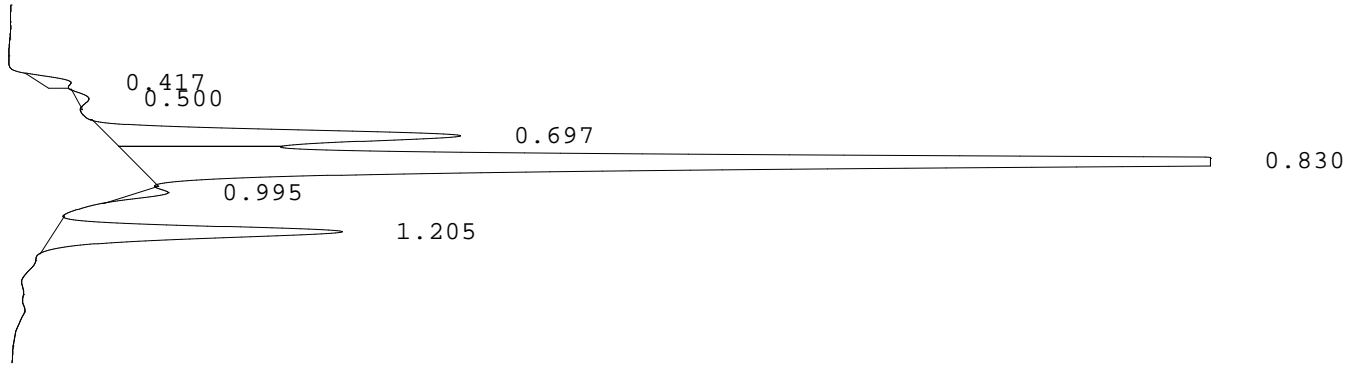

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.417	F 0.50	1.1%	9585	
2	0.500	F 0.60	0.5%	4469	
3	0.697	F 0.83	15.7%	142911	Acetylated F peak
4	0.830	F 0.99	69.4%	630057	Consistent with F
5	0.995	F 1.18	1.0%	9299	
6	1.205	A 1.02	12.3%	111585	A peak
Total Area:				907906	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range