


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 1901, Rack A, Plate 1, Well B11, 787763  
[CD252F6426B38CEA] Sep 03, 2025 11:36:44 Pressure = 61 bar (61 to 63)

FA

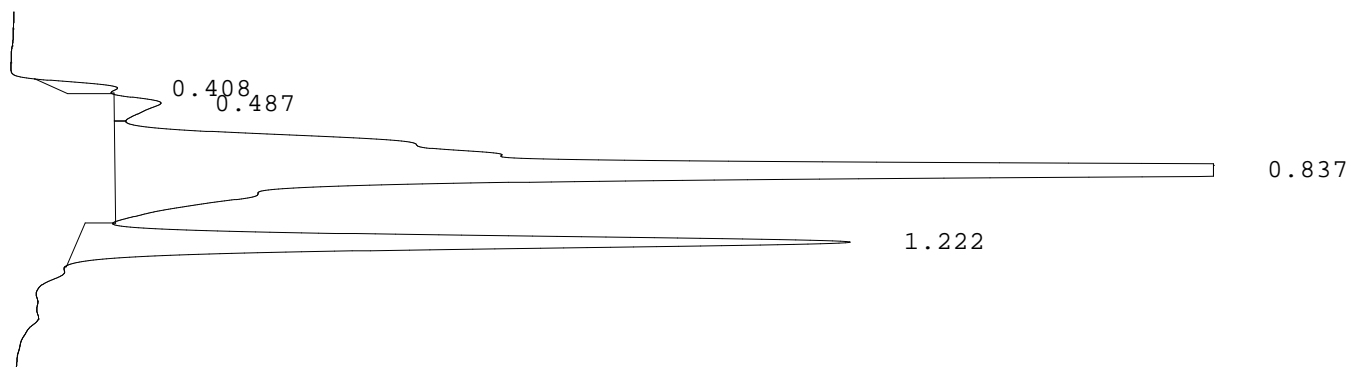

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.408	F 0.49	1.2%	18659	
2	0.487	F 0.58	1.5%	22815	
3	0.837	F 1.00	76.2%	1192700	Consistent with F
4	1.222	A 1.02	21.1%	330049	A peak - REVIEW
Total Area:				1564223	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range