


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2003, Rack A, Plate 1, Well F10, 171349
[9D22FAF17010ACEA] Dec 03, 2025 12:31:08 Pressure = 72 bar (71 to 73)

FA

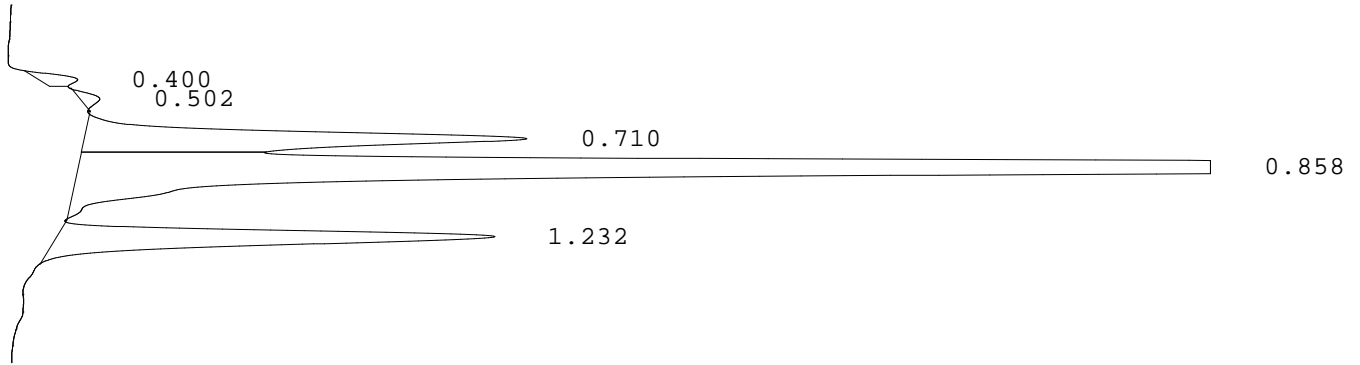

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.47	0.8%	11895	
2	0.502	F 0.58	0.5%	7541	
3	0.710	F 0.83	15.0%	212207	Acetylated F peak
4	0.858	F 1.00	70.0%	991460	Consistent with F
5	1.232	A 1.00	13.6%	192324	A peak

Total Area: 1415427

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range