


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2041, Rack A, Plate 1, Well F06, 488986
[CD72C82306C08E42] Jan 15, 2026 13:01:38 Pressure = 82 bar (81 to 84)

FA

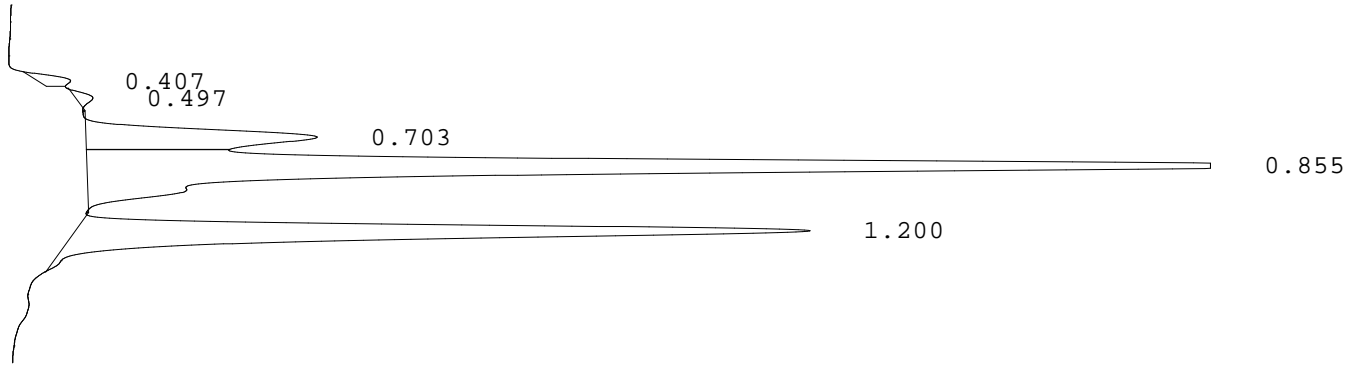

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	0.9%	9802	
2	0.497	F 0.58	0.6%	6196	
3	0.703	F 0.83	11.6%	120362	Acetylated F peak
4	0.855	F 1.01	56.0%	582922	Consistent with F
5	1.200	A 1.01	30.8%	320769	A peak - REVIEW

Total Area: 1040051

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range