


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2113, Rack A, Plate 1, Well D03, 498871
[9C2607D655F6AC42] Apr 07, 2026 12:28:50 Pressure = 59 bar (58 to 60)

FA

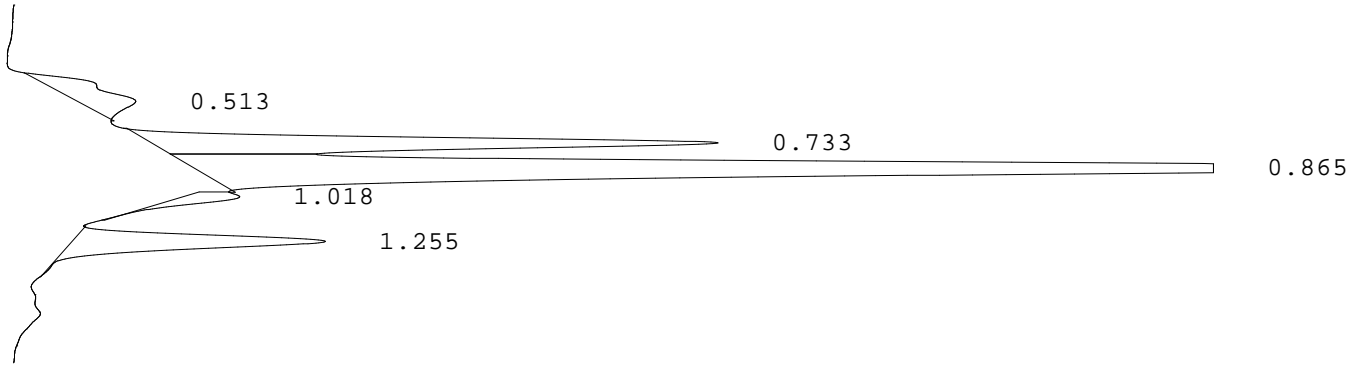

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.513	F 0.59	5.2%	50686	
2	0.733	F 0.84	21.0%	204910	
3	0.865	F 0.99	60.5%	591955	Consistent with F
4	1.018	F 1.16	2.3%	22878	
5	1.255	A 1.00	11.0%	107647	A peak
Total Area:				978076	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range