


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 1974, Rack A, Plate 1, Well D11, 170985  
 [CD77F7BB302DF1B7] Nov 11, 2025 12:44:30 Pressure = 66 bar (66 to 68)

FA

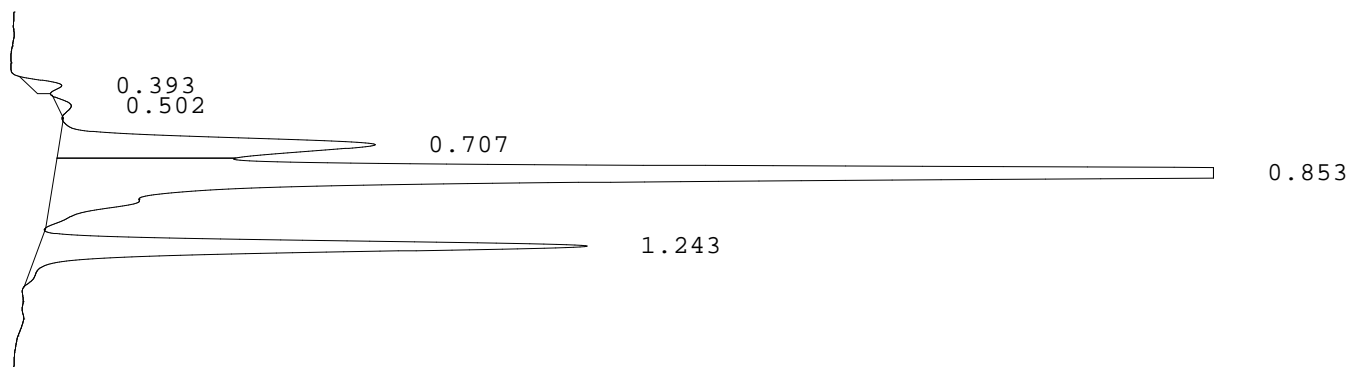

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.393	F 0.45	0.9%	10389	
2	0.502	F 0.58	0.4%	5215	
3	0.707	F 0.82	13.6%	164654	Acetylated F peak
4	0.853	F 0.98	68.4%	828450	Consistent with F
5	1.243	A 1.00	16.7%	202142	A peak
Total Area:				1210850	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range