


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2046, Rack A, Plate 1, Well A06, 488970  
[CD338C6C393D7B97] Jan 16, 2026 10:12:10 Pressure = 83 bar (83 to 85)

FA

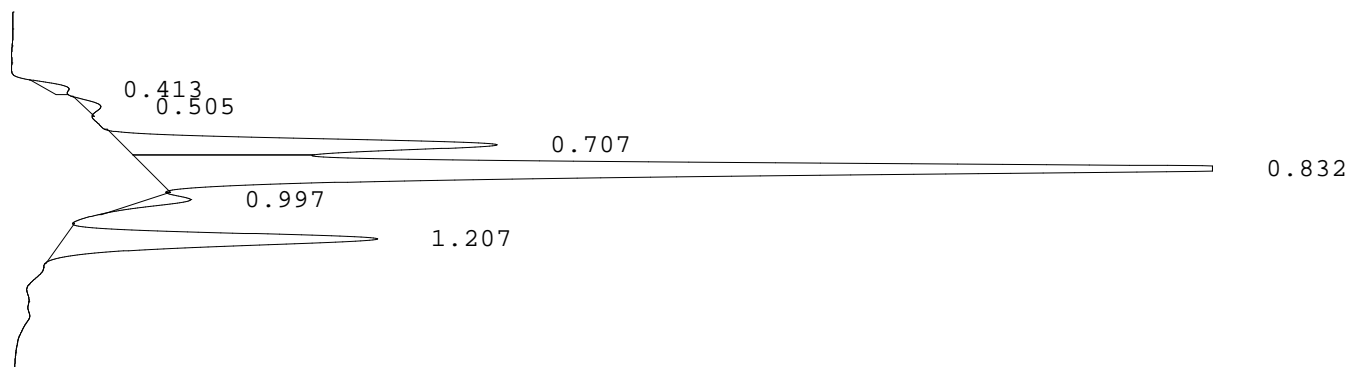

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.413	F 0.49	0.9%	7239	
2	0.505	F 0.60	0.8%	6143	
3	0.707	F 0.84	18.5%	150521	Acetylated F peak
4	0.832	F 0.99	62.1%	504318	Consistent with F
5	0.997	F 1.19	1.9%	15092	
6	1.207	A 1.02	15.9%	129319	A peak
Total Area:				812632	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range