


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2061, Rack A, Plate 1, Well A04, 483341
[DD669F45FE9D5197] Jan 30, 2026 10:07:38 Pressure = 91 bar (91 to 94)

FA

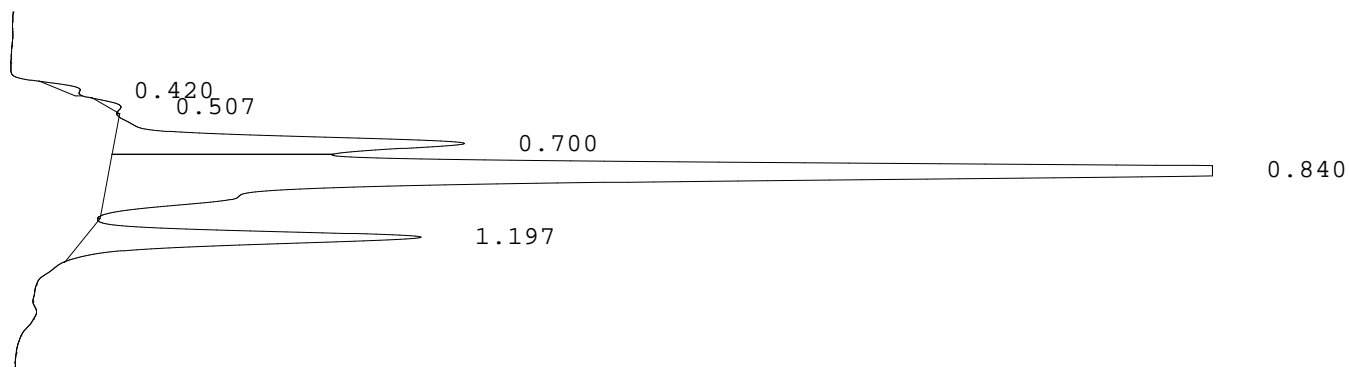

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.420	F 0.50	0.6%	6243	
2	0.507	F 0.61	0.4%	4569	
3	0.700	F 0.84	15.3%	168071	Acetylated F peak
4	0.840	F 1.00	71.0%	782195	Consistent with F
5	1.197	A 1.01	12.7%	140035	A peak

Total Area: 1101113

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range