


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 1948, Rack A, Plate 1, Well D02, 170630  
[DC75580FBE61ACC8] Oct 15, 2025 11:12:09 Pressure = 68 bar (68 to 70)

FA

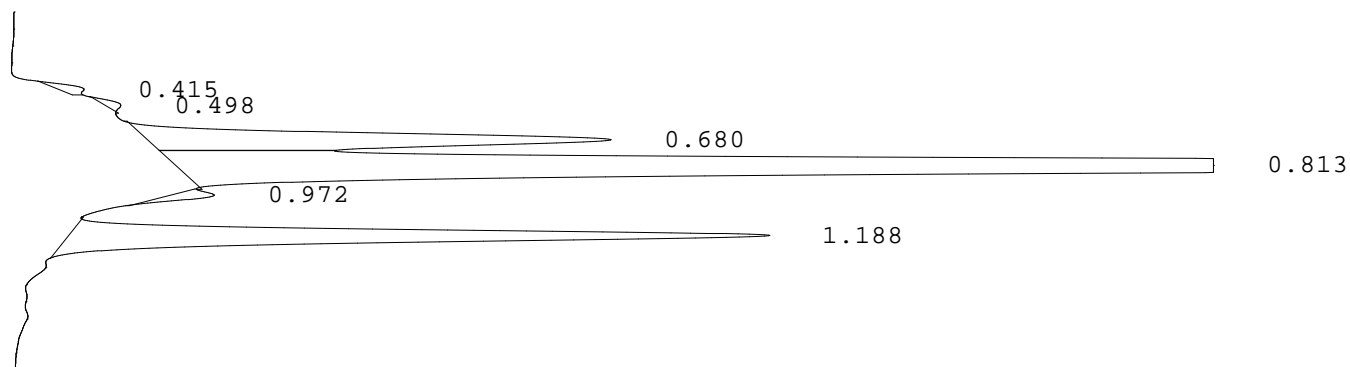

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.415	F 0.50	0.5%	7159	
2	0.498	F 0.60	0.3%	5106	
3	0.680	F 0.82	12.8%	192868	Acetylated F peak
4	0.813	F 0.98	67.8%	1022442	Consistent with F
5	0.972	F 1.17	0.9%	13284	
6	1.188	A 1.00	17.7%	267397	A peak
Total Area:				1508256	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range