


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2095, Rack A, Plate 1, Well H11, 498470  
 [99267F22D3E404E2] Mar 17, 2026 14:45:02 Pressure = 55 bar (55 to 57)

FA

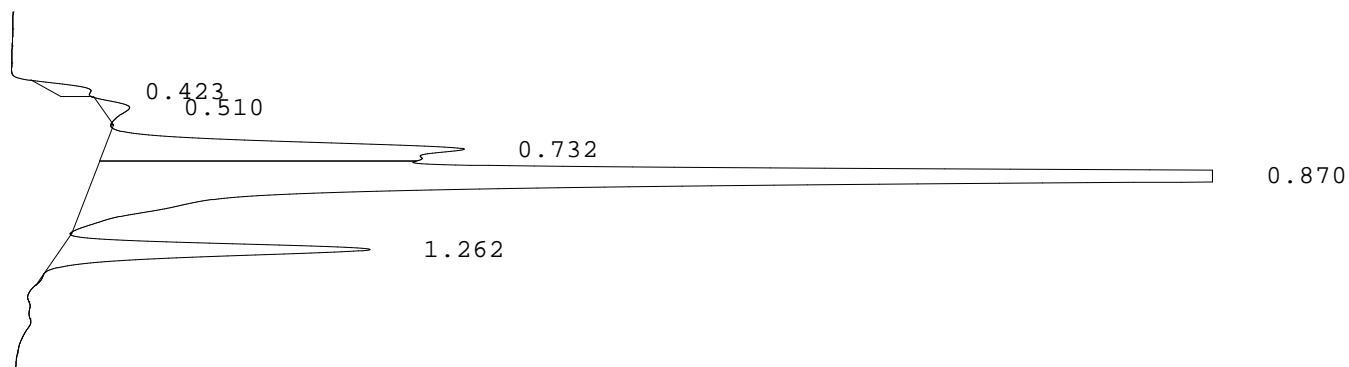

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.423	F 0.47	1.1%	13879	
2	0.510	F 0.57	1.0%	12422	
3	0.732	F 0.81	15.5%	194443	Acetylated F peak
4	0.870	F 0.97	72.6%	910428	Consistent with F
5	1.262	A 1.01	9.8%	122862	A peak
Total Area:				1254034	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range