


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2029, Rack A, Plate 1, Well E11, 490352
 [9933D7EDEF5F599F] Dec 29, 2025 12:53:28 Pressure = 74 bar (74 to 76)

FA

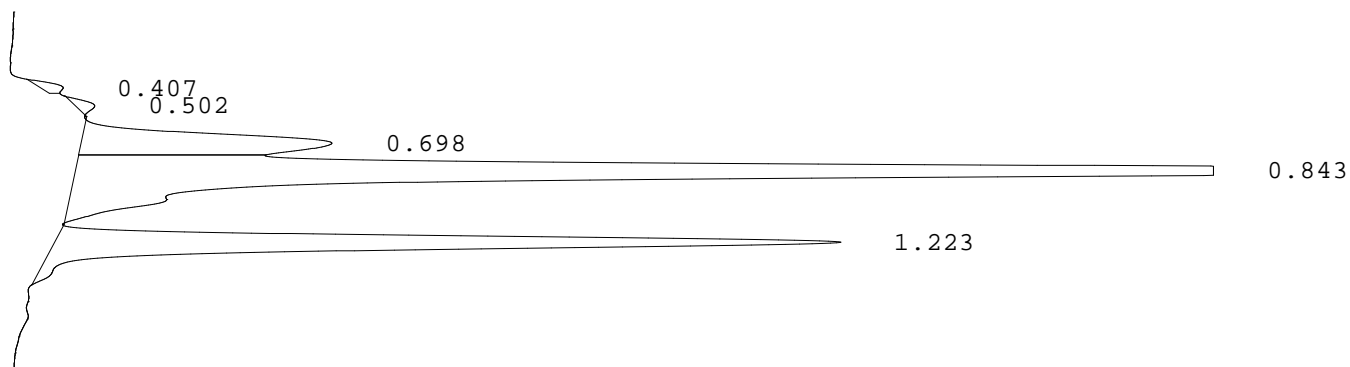

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.47	0.5%	6594	
2	0.502	F 0.58	0.5%	6790	
3	0.698	F 0.81	11.9%	147185	Acetylated F peak
4	0.843	F 0.98	60.7%	752487	Consistent with F
5	1.223	A 1.01	26.3%	326537	A peak - REVIEW
Total Area:				1239593	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range