


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2029, Rack A, Plate 1, Well C10, 490084
 [996797A89000AE62] Dec 29, 2025 12:00:54 Pressure = 74 bar (74 to 77)

FA

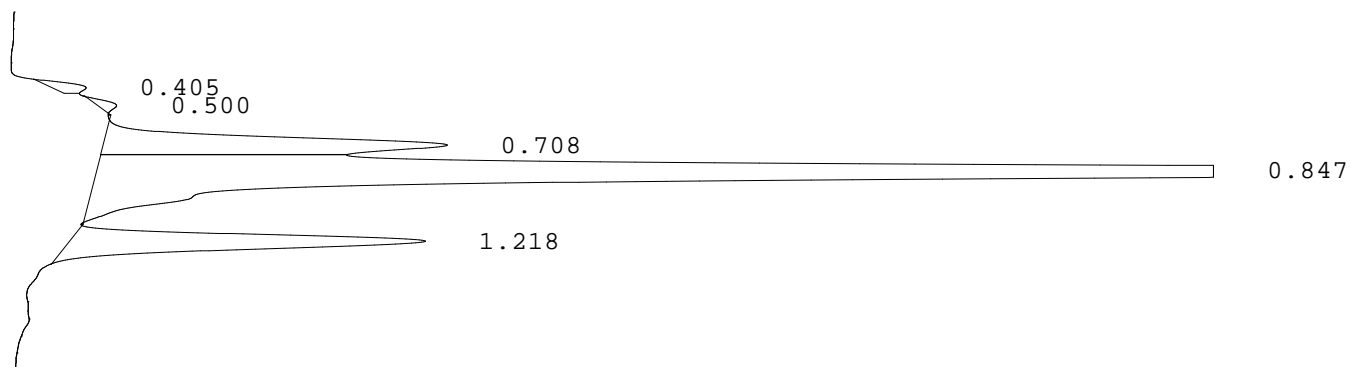

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.47	0.8%	9774	
2	0.500	F 0.59	0.5%	6329	
3	0.708	F 0.83	13.1%	166122	Acetylated F peak
4	0.847	F 0.99	73.0%	922929	Consistent with F
5	1.218	A 1.01	12.6%	159086	A peak
Total Area:				1264240	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range