


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2003, Rack A, Plate 1, Well D10, 484327
[CD36BBF1729A0E6A] Dec 03, 2025 11:40:36 Pressure = 72 bar (72 to 74)

FA

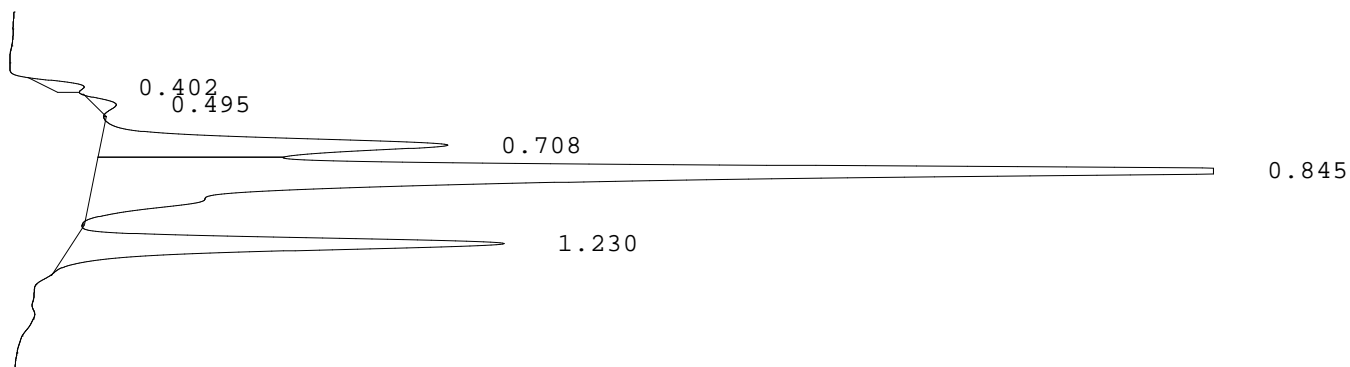

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.402	F 0.47	1.1%	11351	
2	0.495	F 0.57	0.8%	8222	
3	0.708	F 0.82	16.4%	168519	Acetylated F peak
4	0.845	F 0.98	64.3%	658734	Consistent with F
5	1.230	A 1.01	17.4%	177908	A peak
Total Area:				1024734	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range