


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 1893, Rack A, Plate 1, Well A01, 169748
 [CD247D0B1CC6D31D] Aug 27, 2025 09:48:01 Pressure = 64 bar (63 to 65)

FA

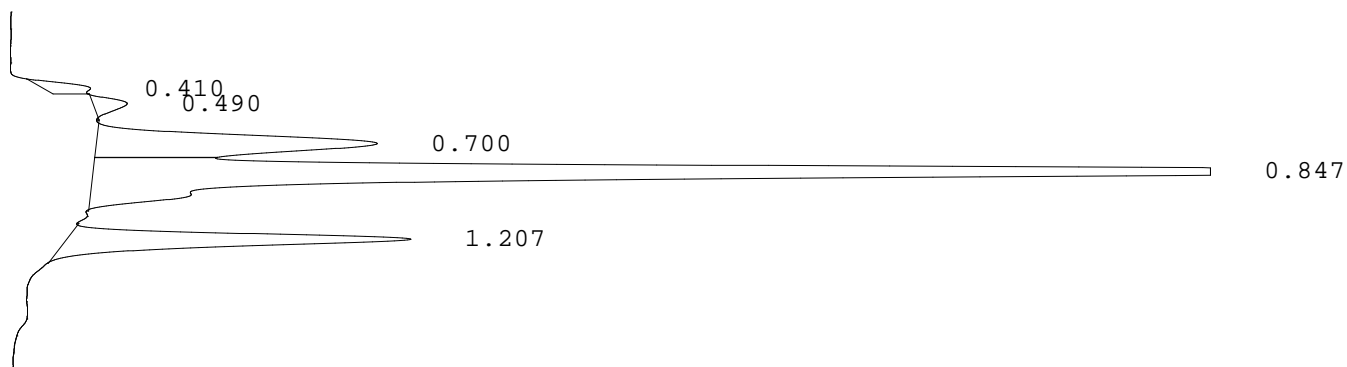

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.410	F 0.49	1.6%	14280	
2	0.490	F 0.58	1.5%	13470	
3	0.700	F 0.83	16.8%	153809	Acetylated F peak
4	0.847	F 1.01	65.6%	602357	Consistent with F
5	1.207	A 1.01	14.6%	134282	A peak
Total Area:				918198	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range