


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2018, Rack A, Plate 1, Well C02, 484359
[9D23D0A15275F917] Dec 15, 2025 10:22:58 Pressure = 75 bar (74 to 77)

FA

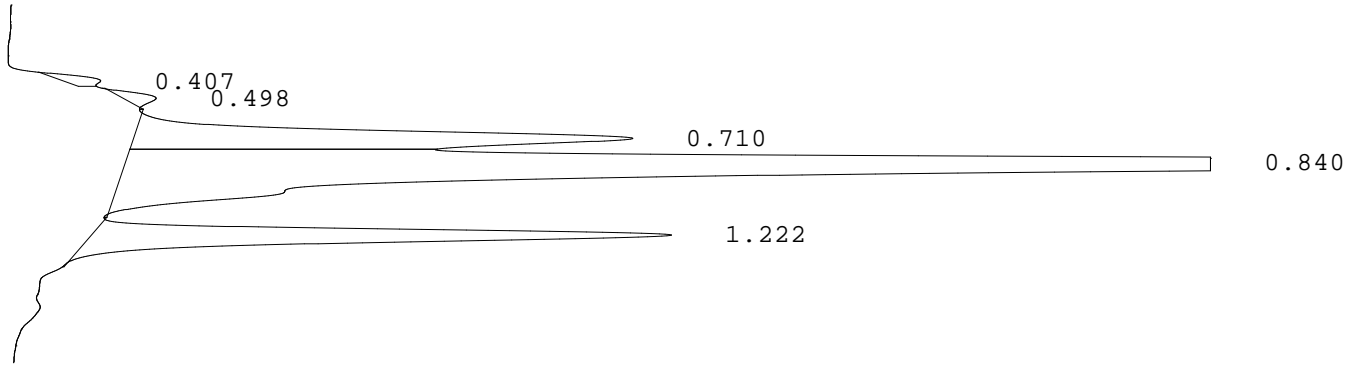

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	0.7%	11051	
2	0.498	F 0.59	0.7%	11975	
3	0.710	F 0.84	15.3%	246621	Acetylated F peak
4	0.840	F 0.99	68.5%	1102925	Consistent with F
5	1.222	A 1.01	14.7%	236444	A peak
Total Area:				1609016	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range