




LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 1795, Rack A, Plate 1, Well C10, 456677  
[8C75FCD0AA4F0EE8] May 14, 2025 11:08:45 Pressure = 57 bar (57 to 59)

FA

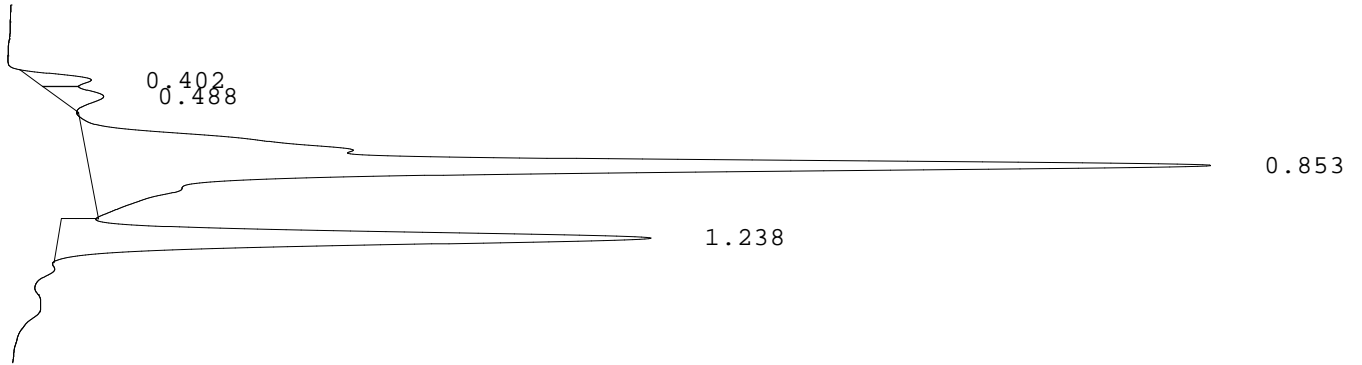

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.402	F 0.47	2.0%	18517	
2	0.488	F 0.57	2.4%	22411	
3	0.853	F 1.00	68.0%	641905	Consistent with F
4	1.238	A 1.01	27.7%	261188	A peak - REVIEW

Total Area: 944021

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range