


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2018, Rack A, Plate 1, Well D10, 486540  
[C86695A1505DFB3F] Dec 15, 2025 11:05:24 Pressure = 73 bar (73 to 75)

FA

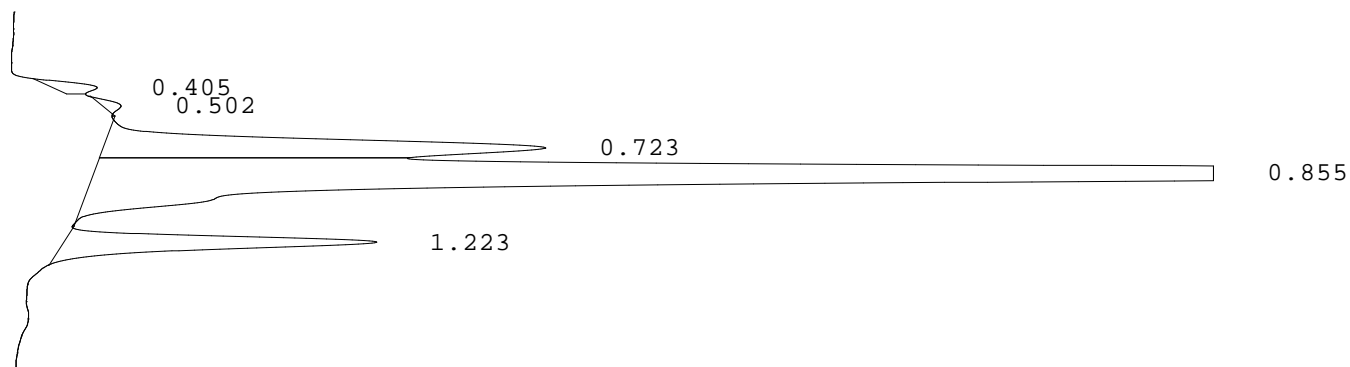

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.47	0.9%	13242	
2	0.502	F 0.59	0.5%	6594	
3	0.723	F 0.84	15.9%	224806	Acetylated F peak
4	0.855	F 1.00	74.0%	1048368	Consistent with F
5	1.223	A 1.00	8.7%	123347	A peak
Total Area:				1416357	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range