


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2018, Rack A, Plate 1, Well F11, 483324
[8C22D1A150F7593D] Dec 15, 2025 11:57:57 Pressure = 72 bar (72 to 74)

FA

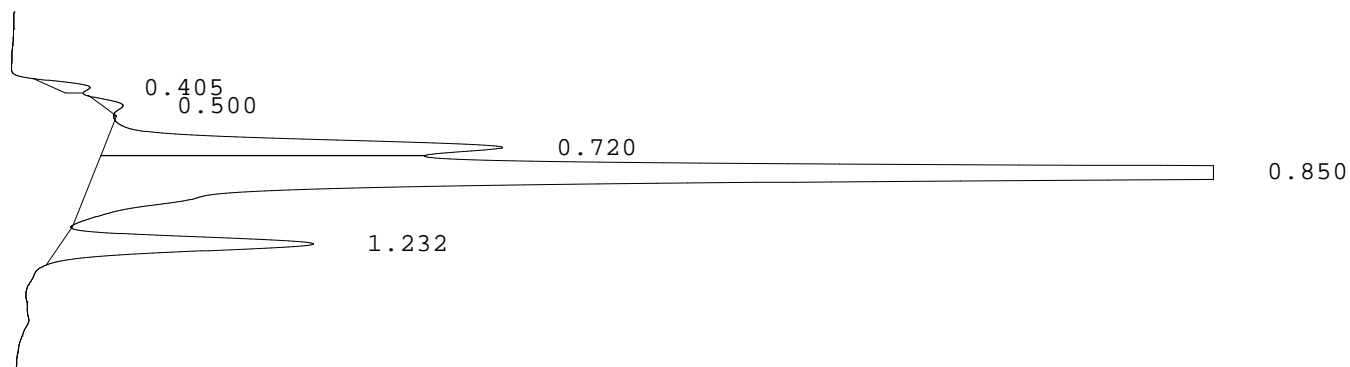

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.405	F 0.47	0.8%	10807	
2	0.500	F 0.58	0.5%	7366	
3	0.720	F 0.84	13.6%	186258	Acetylated F peak
4	0.850	F 0.99	77.0%	1057073	Consistent with F
5	1.232	A 1.01	8.1%	111866	A peak
Total Area:				1373370	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range