


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 2061, Rack A, Plate 1, Well E11, 489190  
[8C36CE05F63F5197] Jan 30, 2026 12:02:50 Pressure = 90 bar (89 to 92)

FA

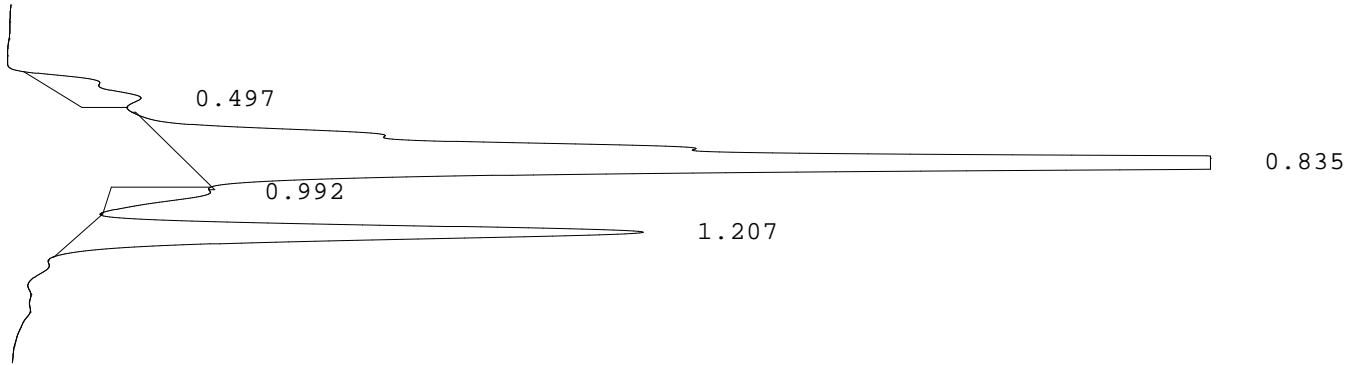

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.497	F 0.59	3.7%	54763	
2	0.835	F 0.99	75.7%	1107470	Consistent with F
3	0.992	F 1.17	3.2%	46176	
4	1.207	A 1.01	17.4%	255024	A peak
Total Area:				1463433	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range