


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2018, Rack A, Plate 1, Well B03, 171471
 [C97380A15257D9BF] Dec 15, 2025 10:00:44 Pressure = 75 bar (74 to 77)

FA

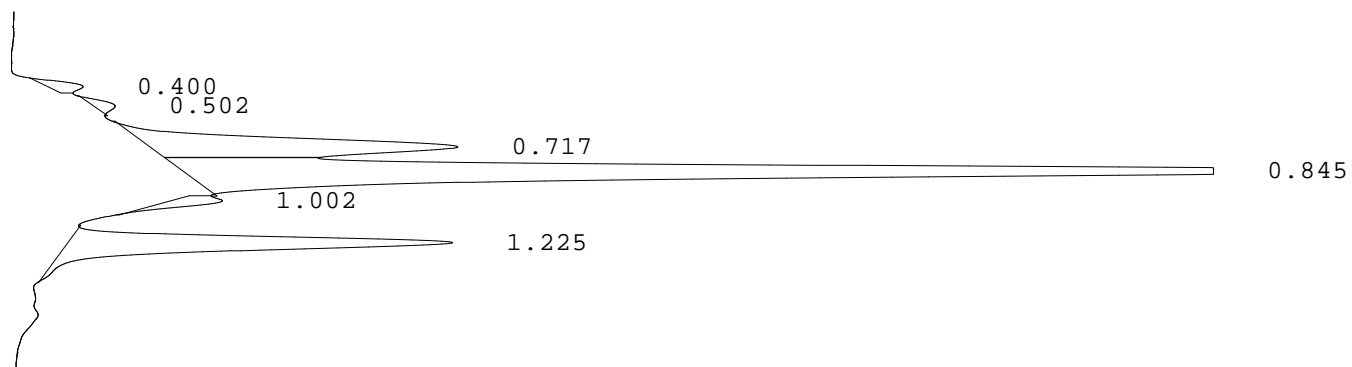

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.400	F 0.47	1.2%	10255	
2	0.502	F 0.59	0.9%	7628	
3	0.717	F 0.84	18.0%	154577	
4	0.845	F 0.99	58.9%	505981	Consistent with F
5	1.002	F 1.18	2.1%	17976	
6	1.225	A 1.01	18.9%	162157	A peak
Total Area:				858574	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range