


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2204, Rack A, Plate 1, Well E03, 495913
[DD3898E96F351115] Jul 23, 2026 11:54:11

Pressure = 93 bar (93 to 95)

FA

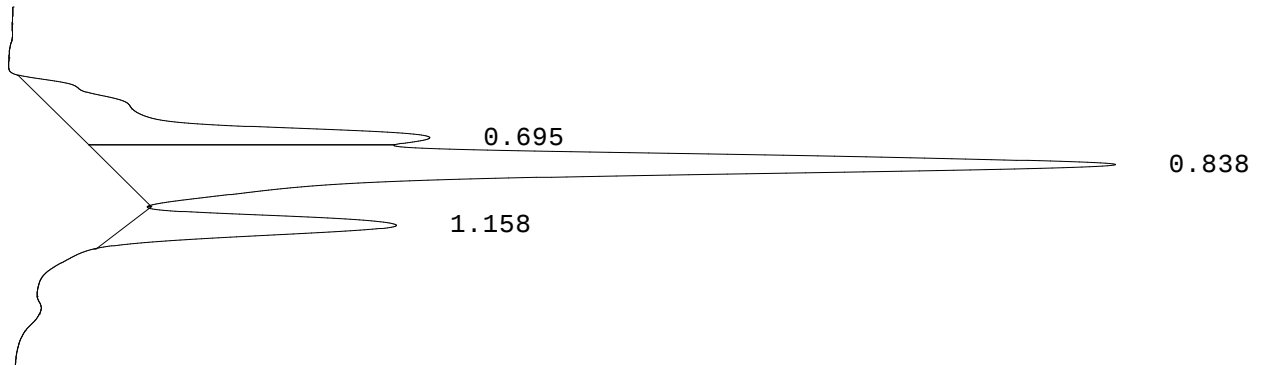

PEAK	RT	REL	RT	% CONC	AREA	COMMENT
1	0.695	F	0.84	22.5%	260275	
2	0.838	F	1.01	63.9%	739716	Consistent with F
3	1.158	A	1.00	13.7%	158086	A peak
Total Area: 1158077						

Codes: 1) Wide A peak
2) Area of A peak < 80%
3) Peak area greater than expected
4) Peak after A2
5) A1c > 10%
6) HbF or variant present
7) Total sample area too small/big
8) A2 is not within normal range