


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2029, Rack A, Plate 1, Well E08, 490087
 [892693A890A20442] Dec 29, 2025 12:45:22 Pressure = 74 bar (74 to 76)

FA

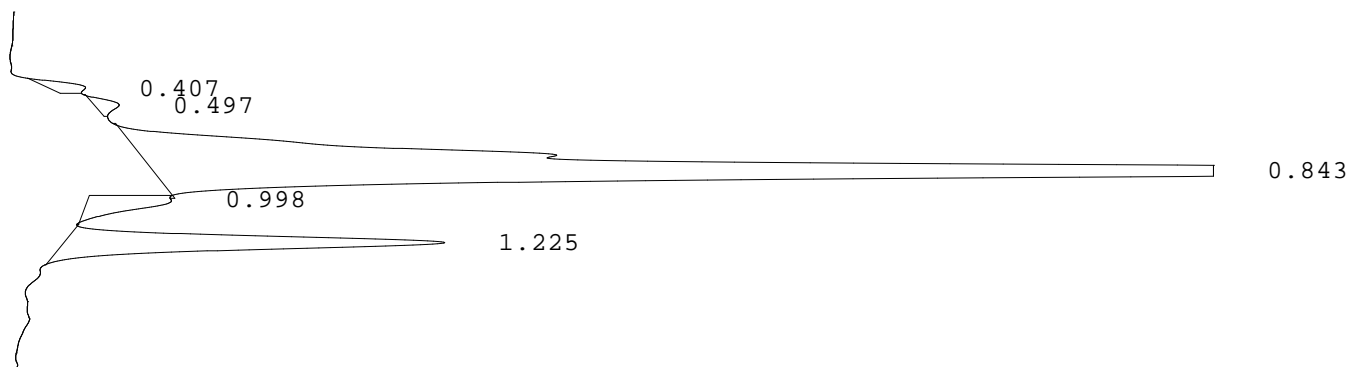

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.407	F 0.48	1.0%	11522	
2	0.497	F 0.58	0.9%	9752	
3	0.843	F 0.99	80.7%	912759	Consistent with F
4	0.998	F 1.17	3.5%	39180	
5	1.225	A 1.01	13.9%	157159	A peak
				Total Area: 1130372	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range