


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2121, Rack A, Plate 1, Well A12, 498285
 [DD730343095C8E6A] Apr 13, 2026 10:53:40 Pressure = 58 bar (57 to 59)

FA

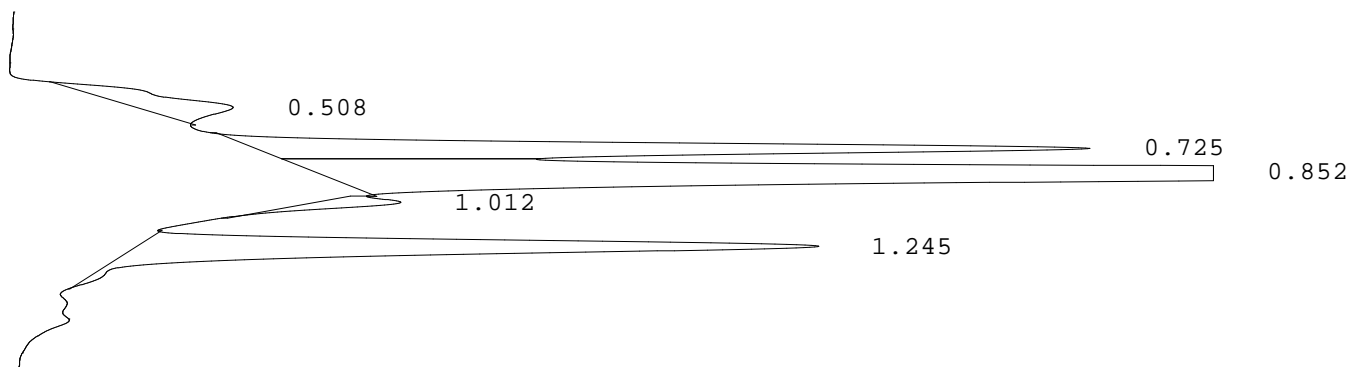

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.508	F 0.59	4.5%	69458	
2	0.725	F 0.84	19.3%	299495	
3	0.852	F 0.98	54.6%	845473	Consistent with F
4	1.012	F 1.17	1.9%	30074	
5	1.245	A 1.00	19.6%	303714	A peak
Total Area:				1548214	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range