


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2003, Rack A, Plate 1, Well D02, 484322
 [DD23EAA4276F5197] Dec 03, 2025 11:24:26 Pressure = 73 bar (72 to 74)

FA

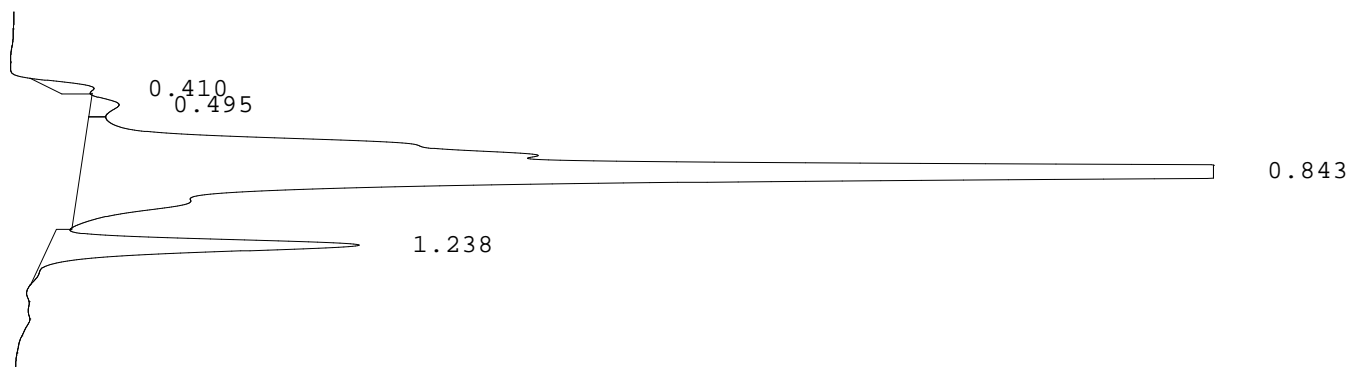

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.410	F 0.48	1.0%	13999	
2	0.495	F 0.57	0.9%	13358	
3	0.843	F 0.98	89.3%	1310728	Consistent with F
4	1.238	A 1.02	8.8%	129308	A peak
Total Area:				1467393	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range