


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2003, Rack A, Plate 1, Well F05, 484325
[DC63BAF1701824E2] Dec 03, 2025 12:21:02 Pressure = 72 bar (72 to 74)

FA

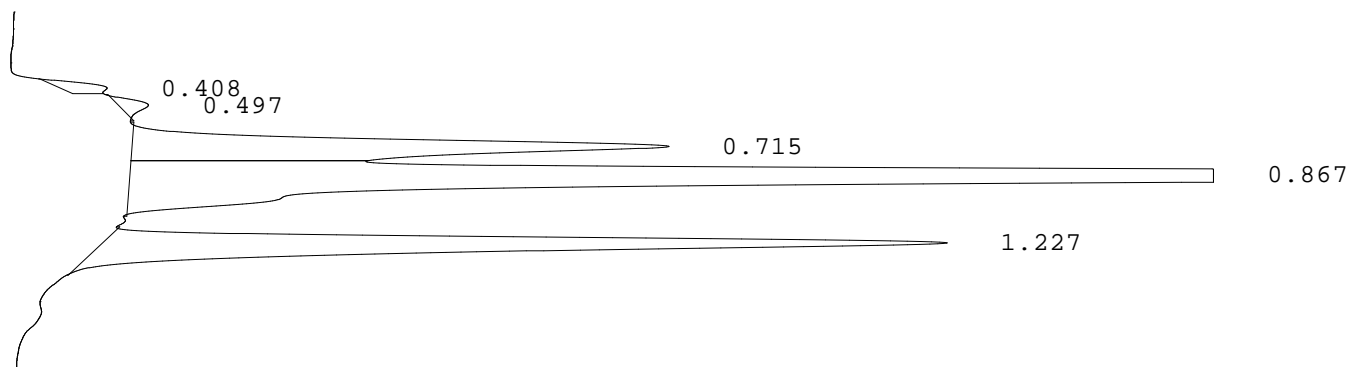

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.408	F 0.48	0.9%	14440	
2	0.497	F 0.58	0.7%	12204	
3	0.715	F 0.83	16.1%	266026	Acetylated F peak
4	0.867	F 1.01	60.1%	990478	Consistent with F
5	1.227	A 0.99	22.2%	365640	A peak - REVIEW

Total Area: 1648788

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range