


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2029, Rack A, Plate 1, Well E09, 490088
[9D7293A890A286C0] Dec 29, 2025 12:47:23 Pressure = 74 bar (74 to 76)

FA

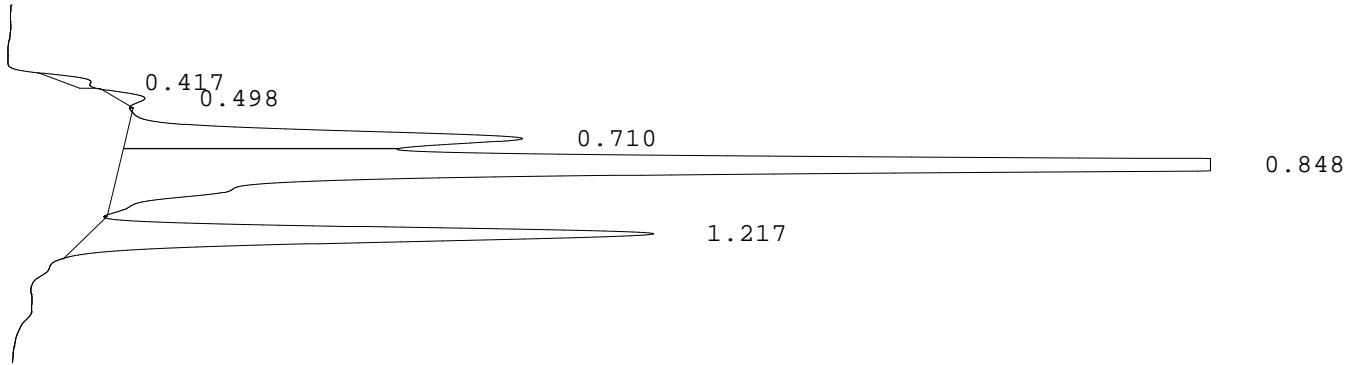

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.417	F 0.49	0.7%	9610	
2	0.498	F 0.58	0.7%	9630	
3	0.710	F 0.83	14.1%	198001	Acetylated F peak
4	0.848	F 0.99	66.0%	926650	Consistent with F
5	1.217	A 1.01	18.5%	260102	A peak
Total Area:				1403993	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range