


LABORATORIO PREGEN  
 Carrera 15a No 106-42  
 BOGOTA

Batch 2022, Rack A, Plate 1, Well H09, 490071  
 [C973D0C2DD22AC40] Dec 19, 2025 13:17:55 Pressure = 73 bar (72 to 74)

FA

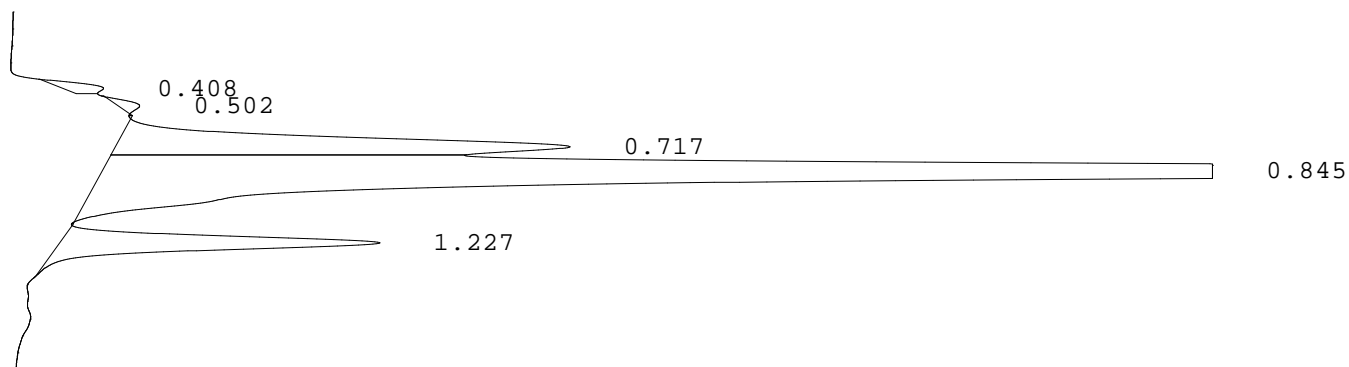

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.408	F 0.48	0.8%	12158	
2	0.502	F 0.59	0.5%	7736	
3	0.717	F 0.84	14.8%	229359	Acetylated F peak
4	0.845	F 0.99	75.0%	1161305	Consistent with F
5	1.227	A 1.01	8.9%	137124	A peak
Total Area:				1547682	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range