


LABORATORIO PREGEN  
Carrera 15a No 106-42  
BOGOTA

Batch 1884, Rack A, Plate 1, Well C03, 169632  
[CD707715D4A6F3B7] Aug 13, 2025 11:35:58 Pressure = 61 bar (60 to 62)

FA

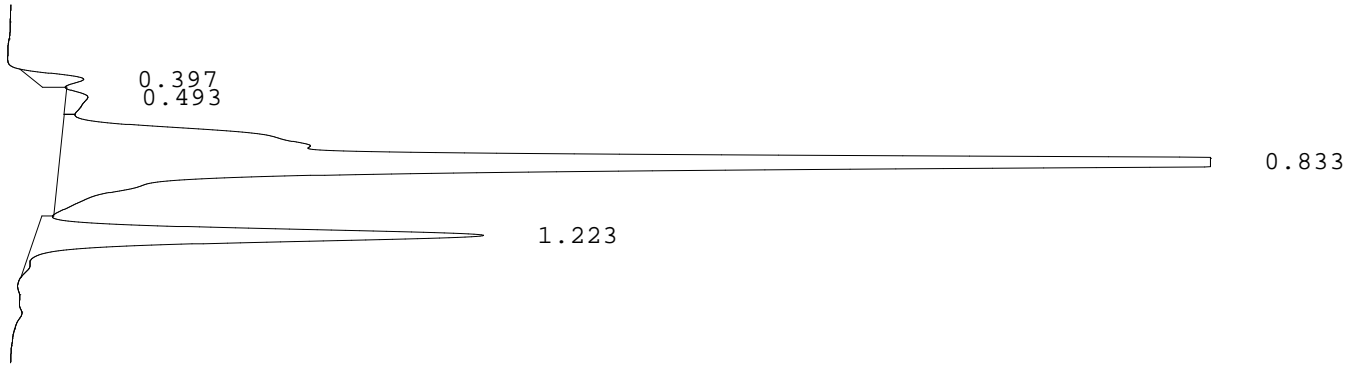

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.397	F 0.47	1.5%	16720	
2	0.493	F 0.59	1.1%	12133	
3	0.833	F 0.99	80.3%	892459	Consistent with F
4	1.223	A 1.02	17.1%	189790	A peak
Total Area:				1111102	

- Codes:
- 1) Wide A peak
  - 2) Area of A peak < 80%
  - 3) Peak area greater than expected
  - 4) Peak after A2
  - 5) Alc > 10%
  - 6) HbF or variant present
  - 7) Total sample area too small/big
  - 8) A2 is not within normal range