


LABORATORIO PREGEN
 Carrera 15a No 106-42
 BOGOTA

Batch 2008, Rack A, Plate 1, Well D11, 171405
 [C873BE642CBA2EC2] Dec 09, 2025 12:28:42 Pressure = 72 bar (72 to 74)

FA

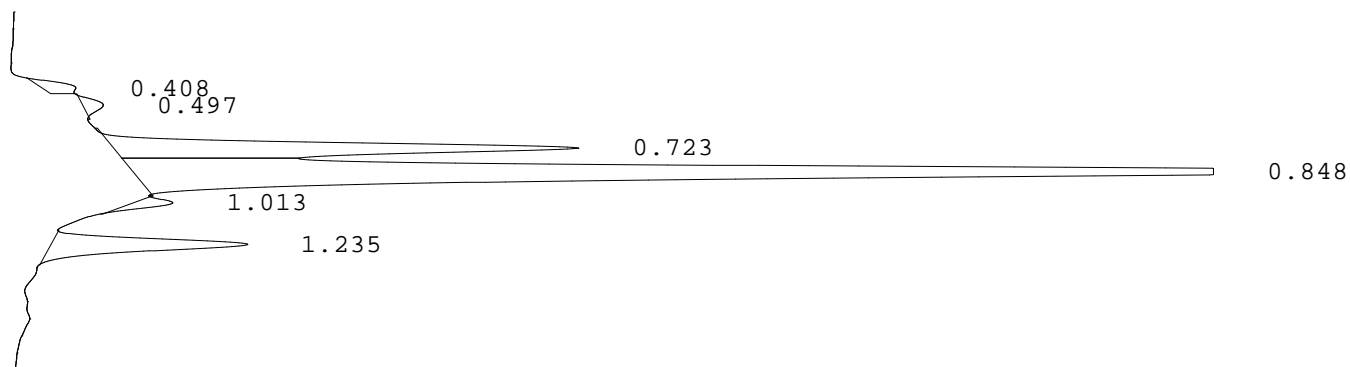

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.408	F 0.47	1.4%	11150	
2	0.497	F 0.57	1.0%	8303	
3	0.723	F 0.83	20.6%	165034	
4	0.848	F 0.98	66.3%	531606	Consistent with F
5	1.013	F 1.17	1.5%	11865	
6	1.235	A 1.02	9.2%	73839	A peak
Total Area:				801797	

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range