


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2061, Rack A, Plate 1, Well A10, 489301
[8926CF45FEBF591D] Jan 30, 2026 10:19:45 Pressure = 90 bar (90 to 93)

FA

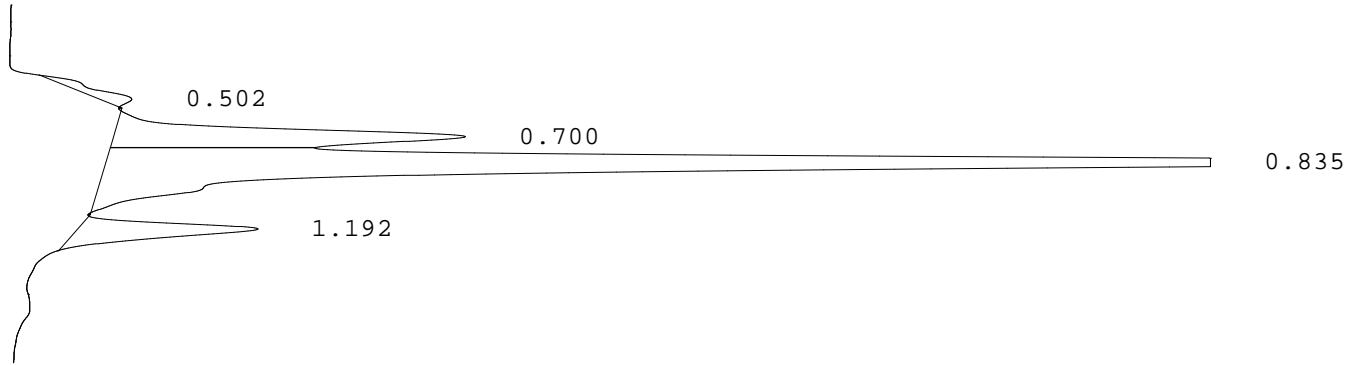

PEAK	RT	REL RT	% CONC	AREA	COMMENT
1	0.502	F 0.60	2.0%	19888	
2	0.700	F 0.84	17.5%	170960	Acetylated F peak
3	0.835	F 1.00	72.5%	708242	Consistent with F
4	1.192	A 1.01	8.0%	78301	A peak

Total Area: 977391

- Codes:
- 1) Wide A peak
 - 2) Area of A peak < 80%
 - 3) Peak area greater than expected
 - 4) Peak after A2
 - 5) Alc > 10%
 - 6) HbF or variant present
 - 7) Total sample area too small/big
 - 8) A2 is not within normal range