


LABORATORIO PREGEN
Carrera 15a No 106-42
BOGOTA

Batch 2194, Rack A, Plate 1, Well G01, 493084
[8C29D14AE9A2E4E2] Jul 09, 2026 12:48:46

FA
Pressure = 80 bar (80 to 83)

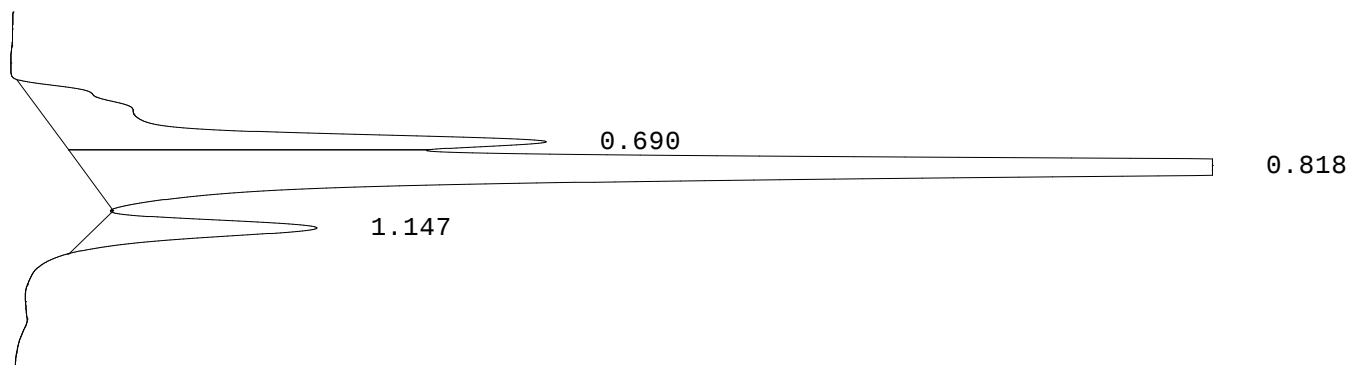

PEAK	RT	REL	RT	% CONC	AREA	COMMENT
1	0.690	F	0.83	20.1%	321703	Acetylated F peak
2	0.818	F	0.99	72.4%	1160192	Consistent with F
3	1.147	A	1.00	7.5%	119667	A peak
Total Area: 1601562						

Codes: 1) Wide A peak
2) Area of A peak < 80%
3) Peak area greater than expected
4) Peak after A2
5) A1c > 10%
6) HbF or variant present
7) Total sample area too small/big
8) A2 is not within normal range